


Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	0000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

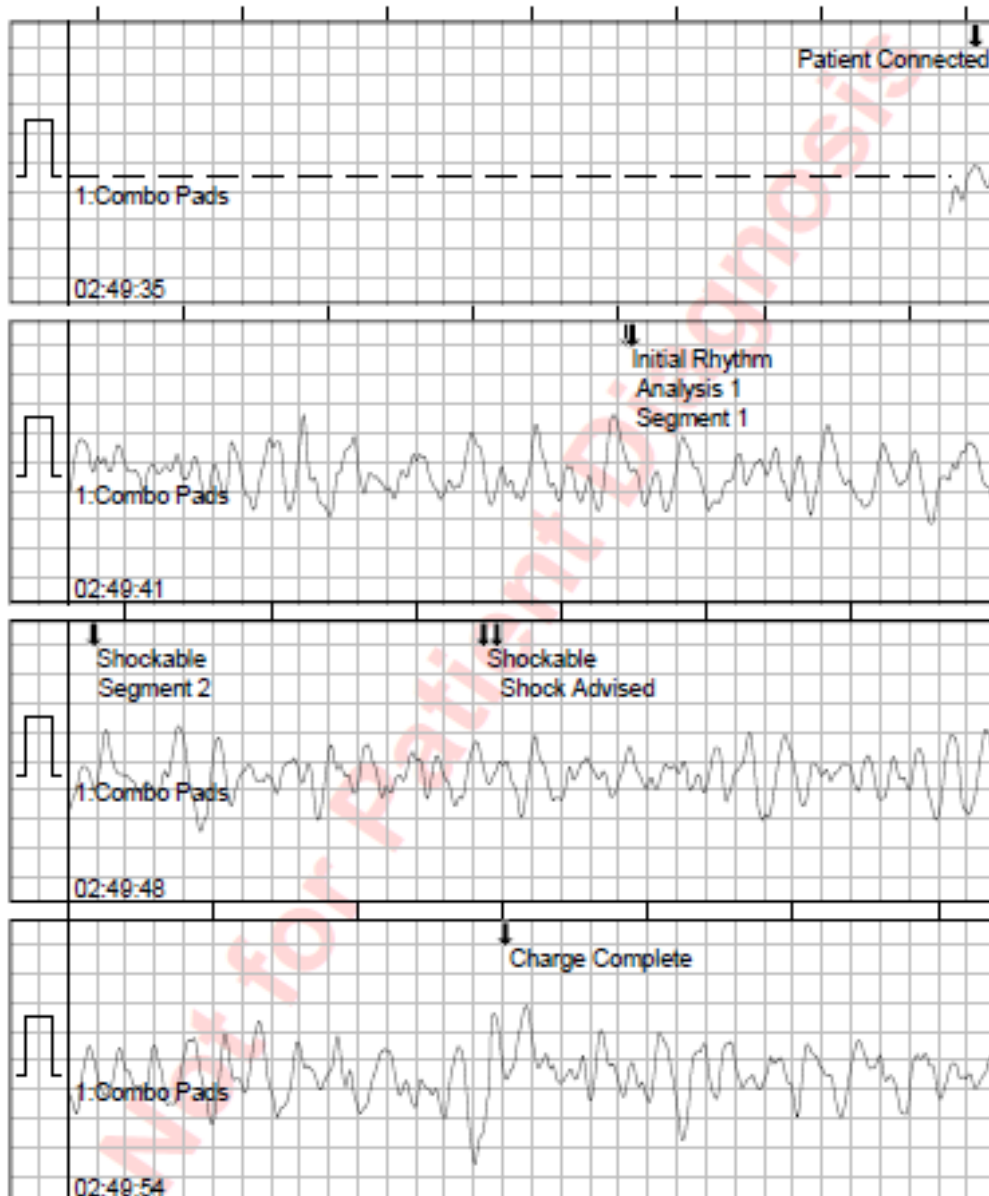

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

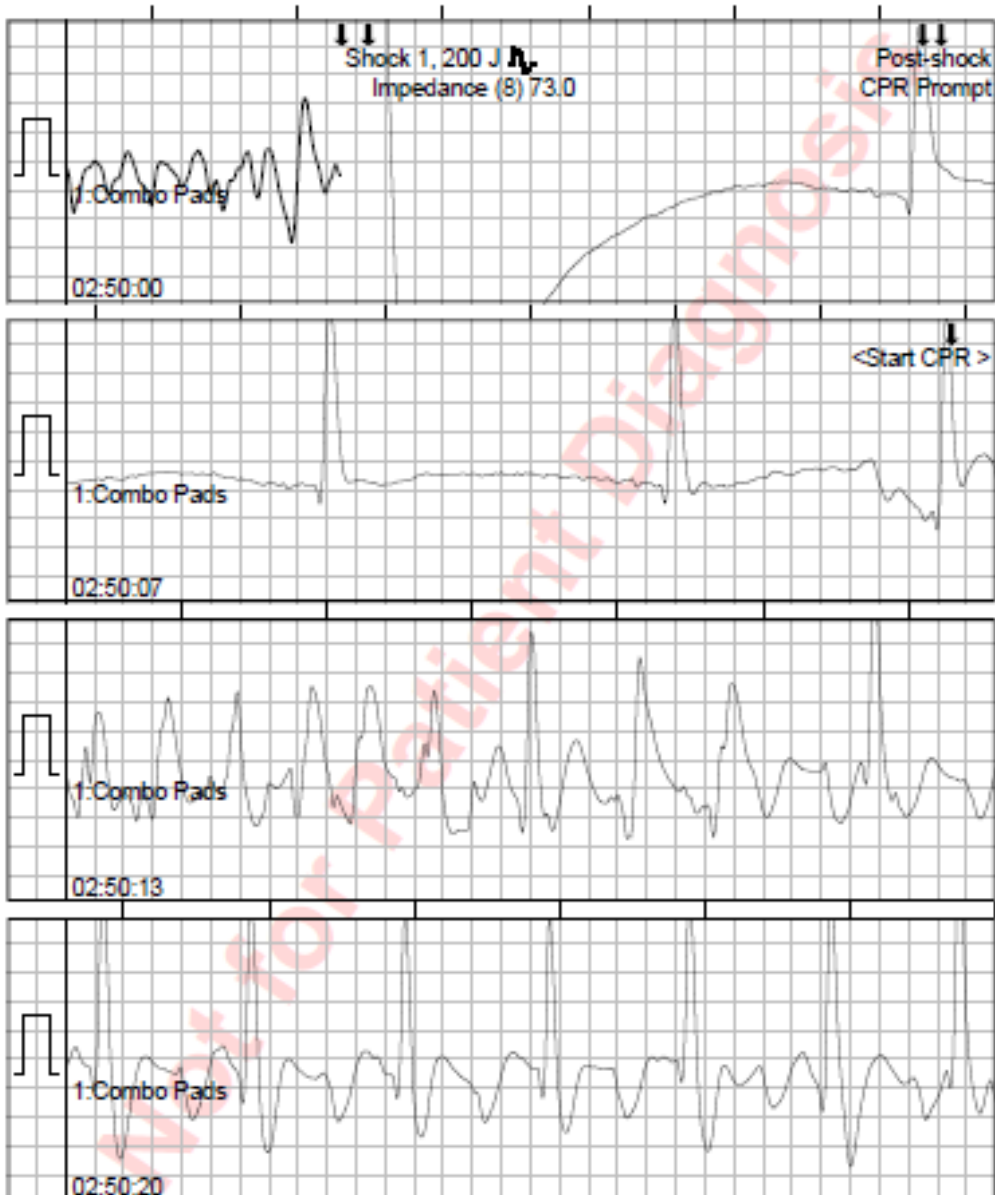

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

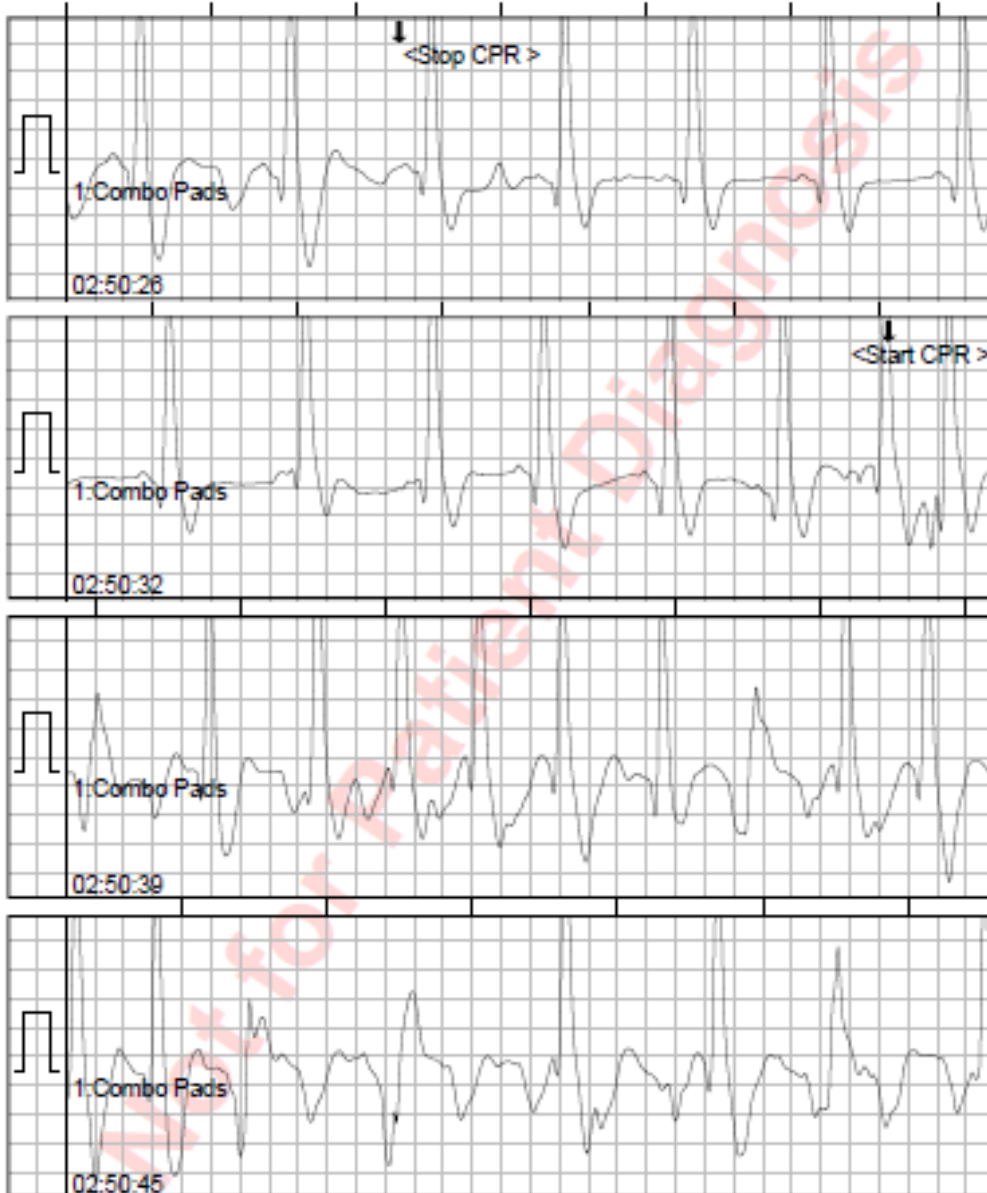

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

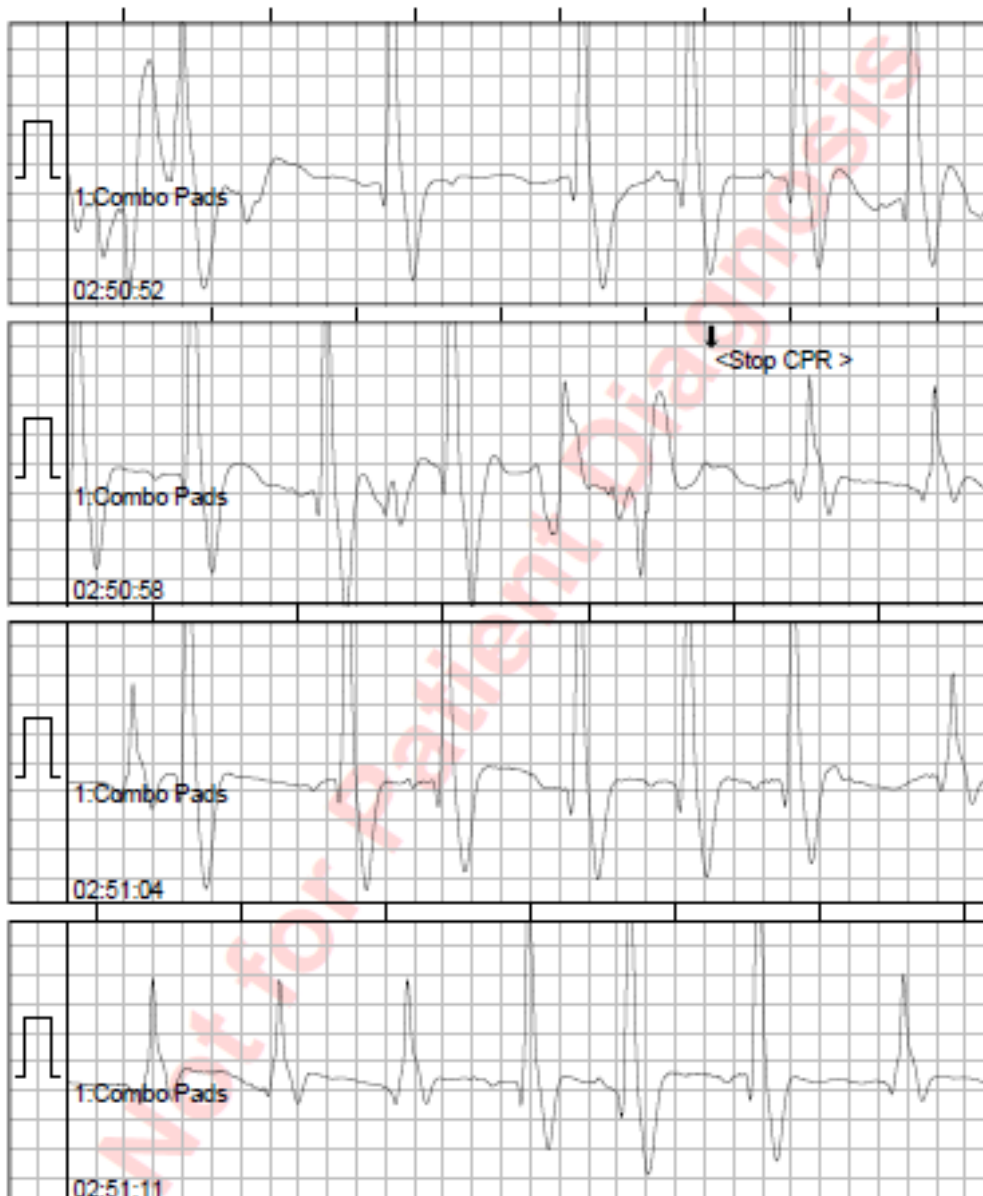

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

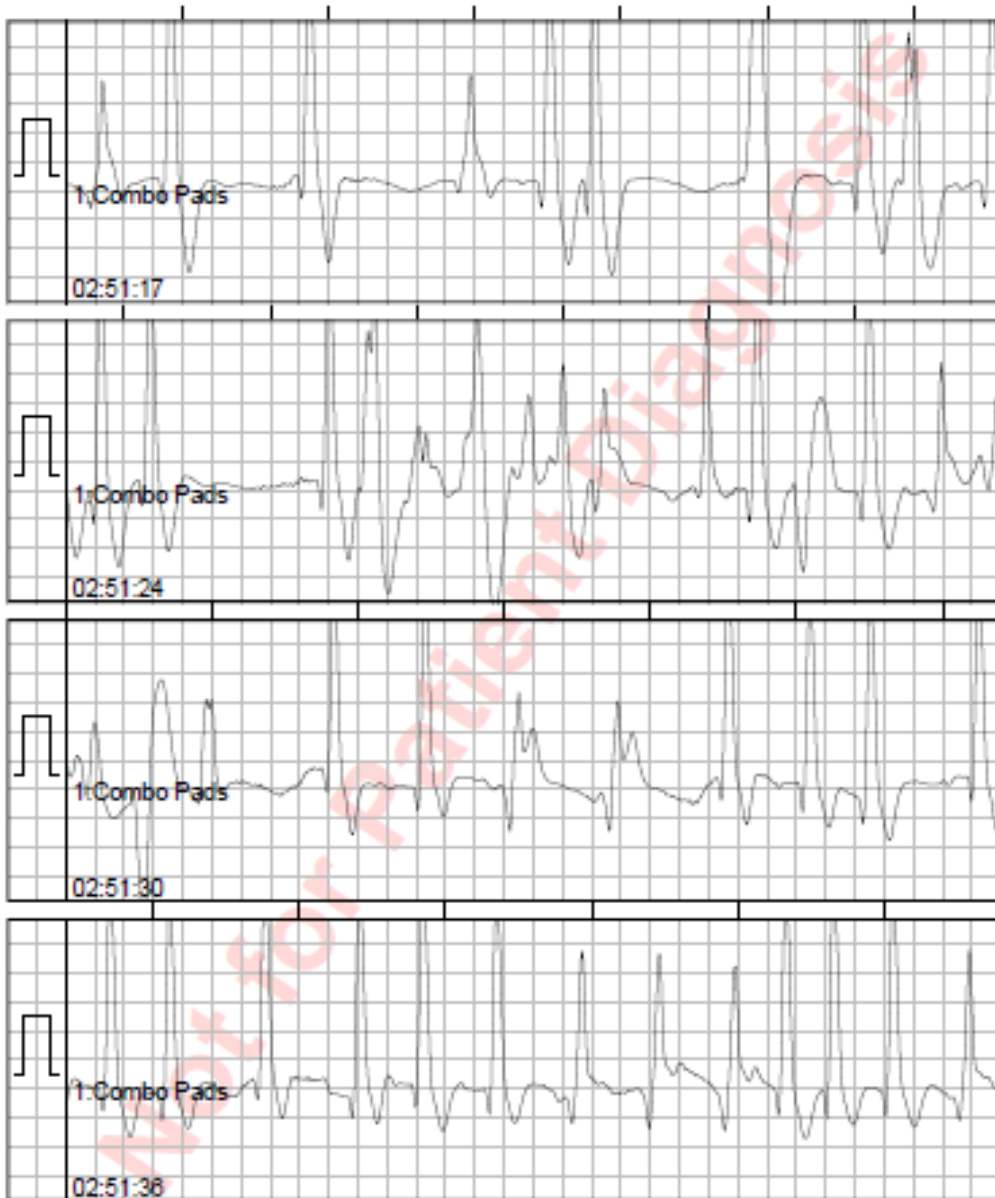

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

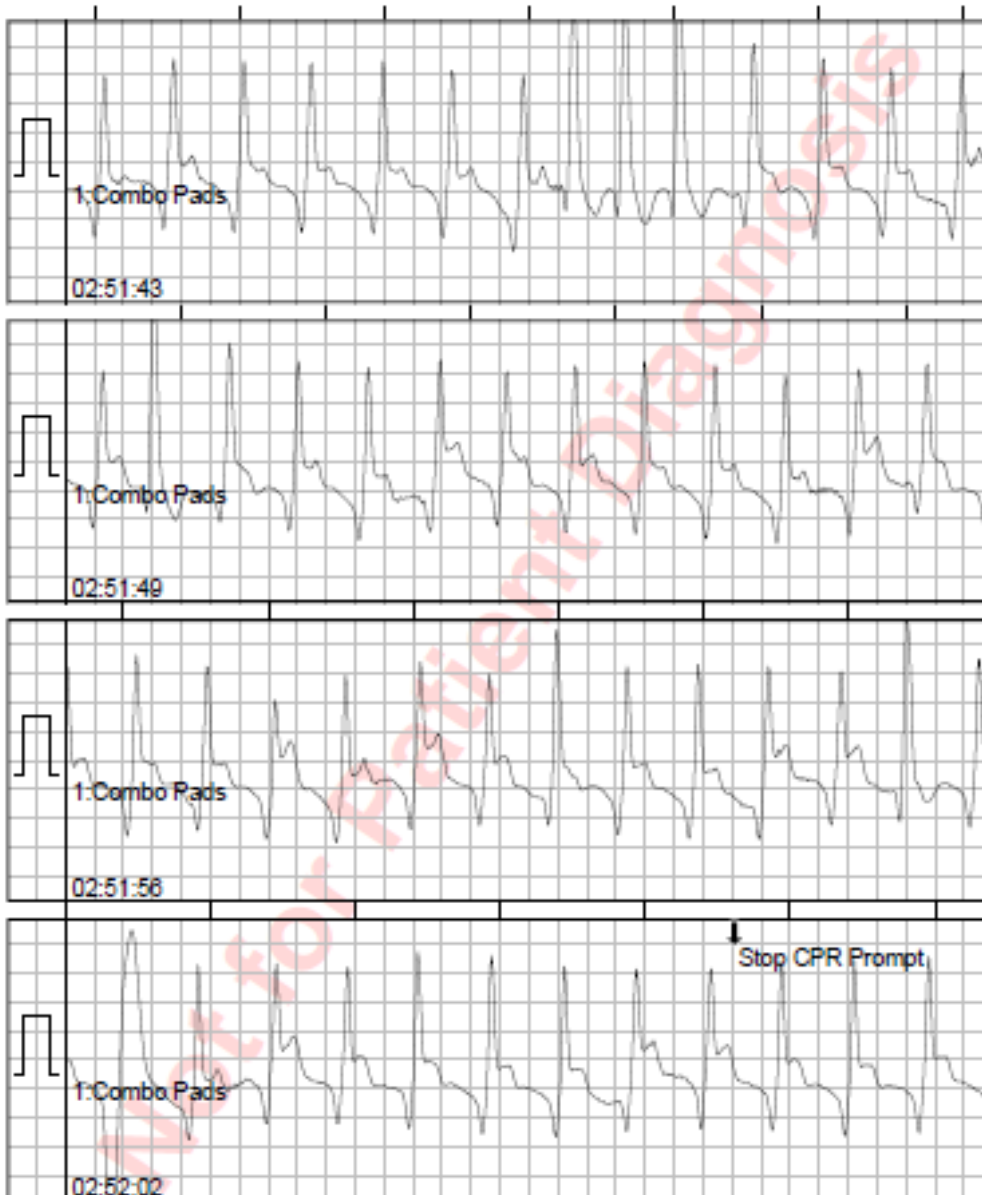

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

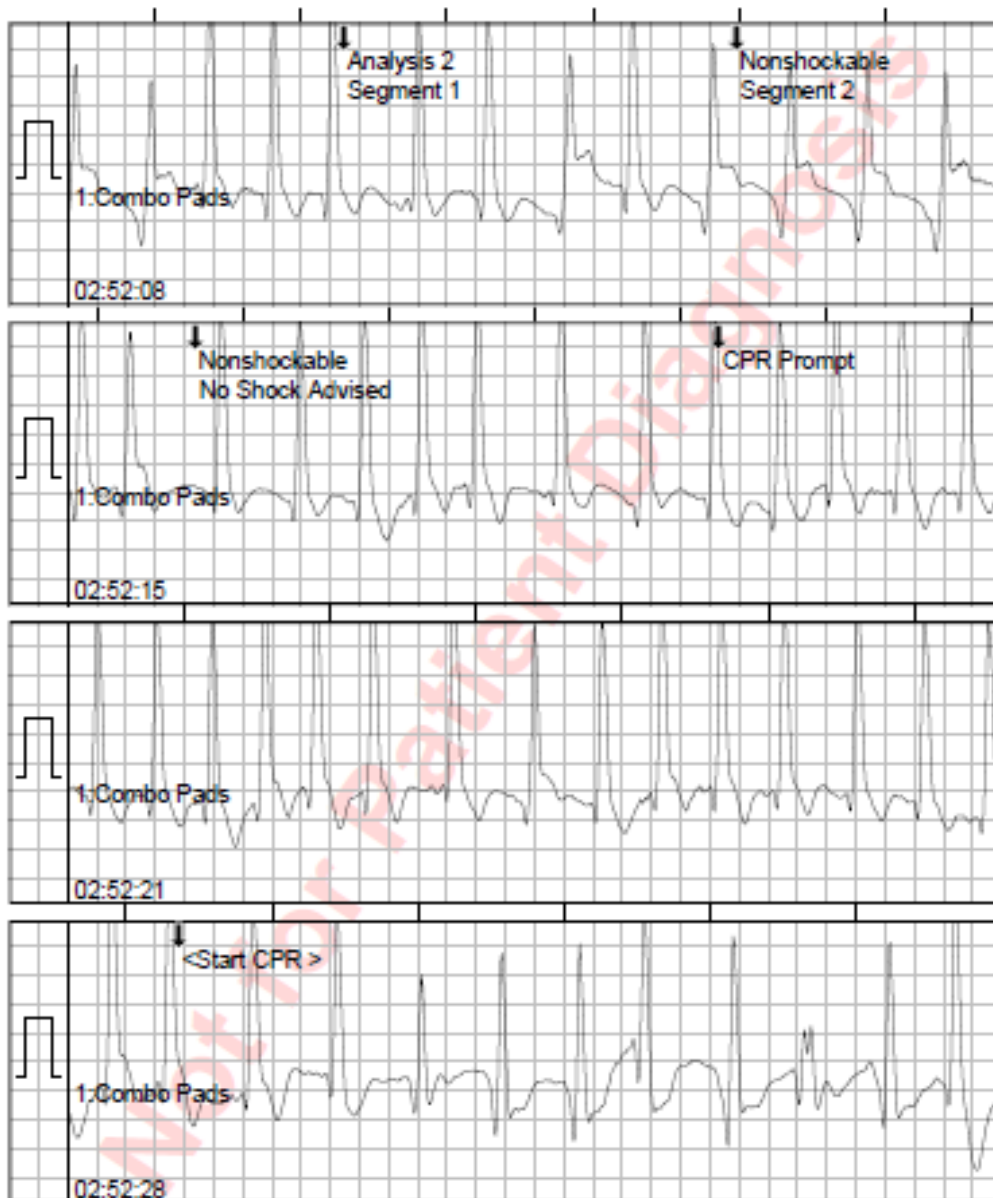

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

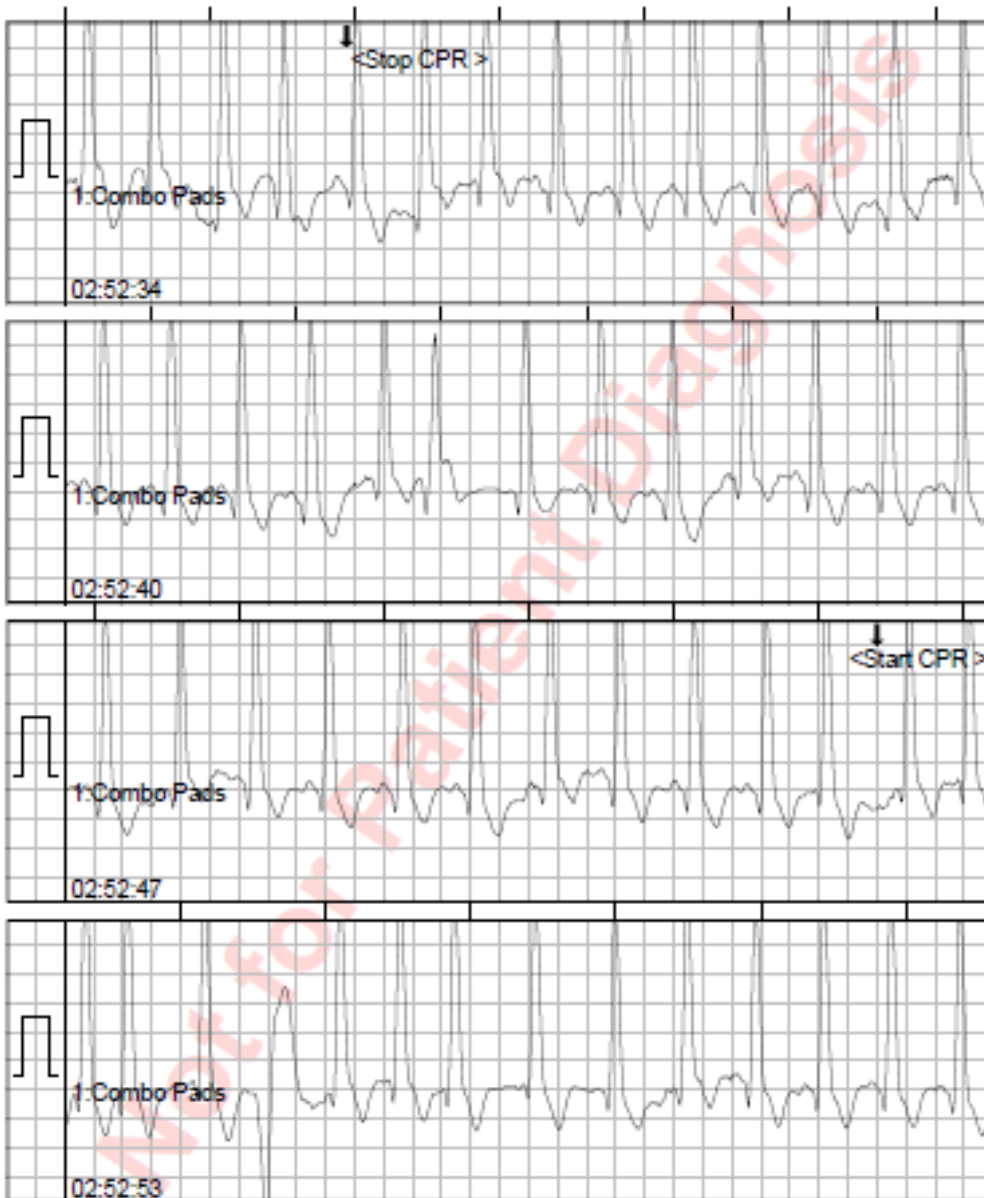

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.

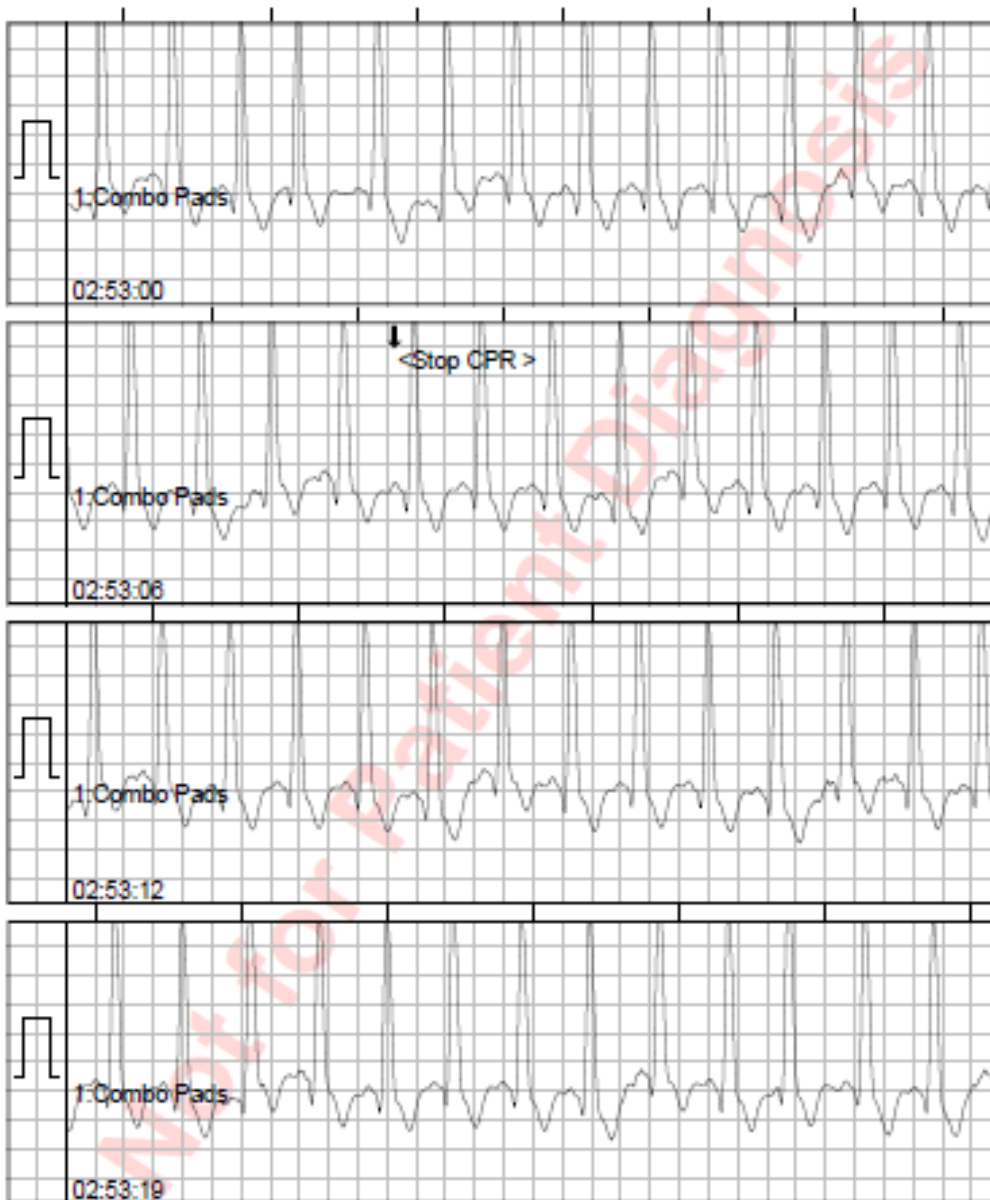

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.



Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.



Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.

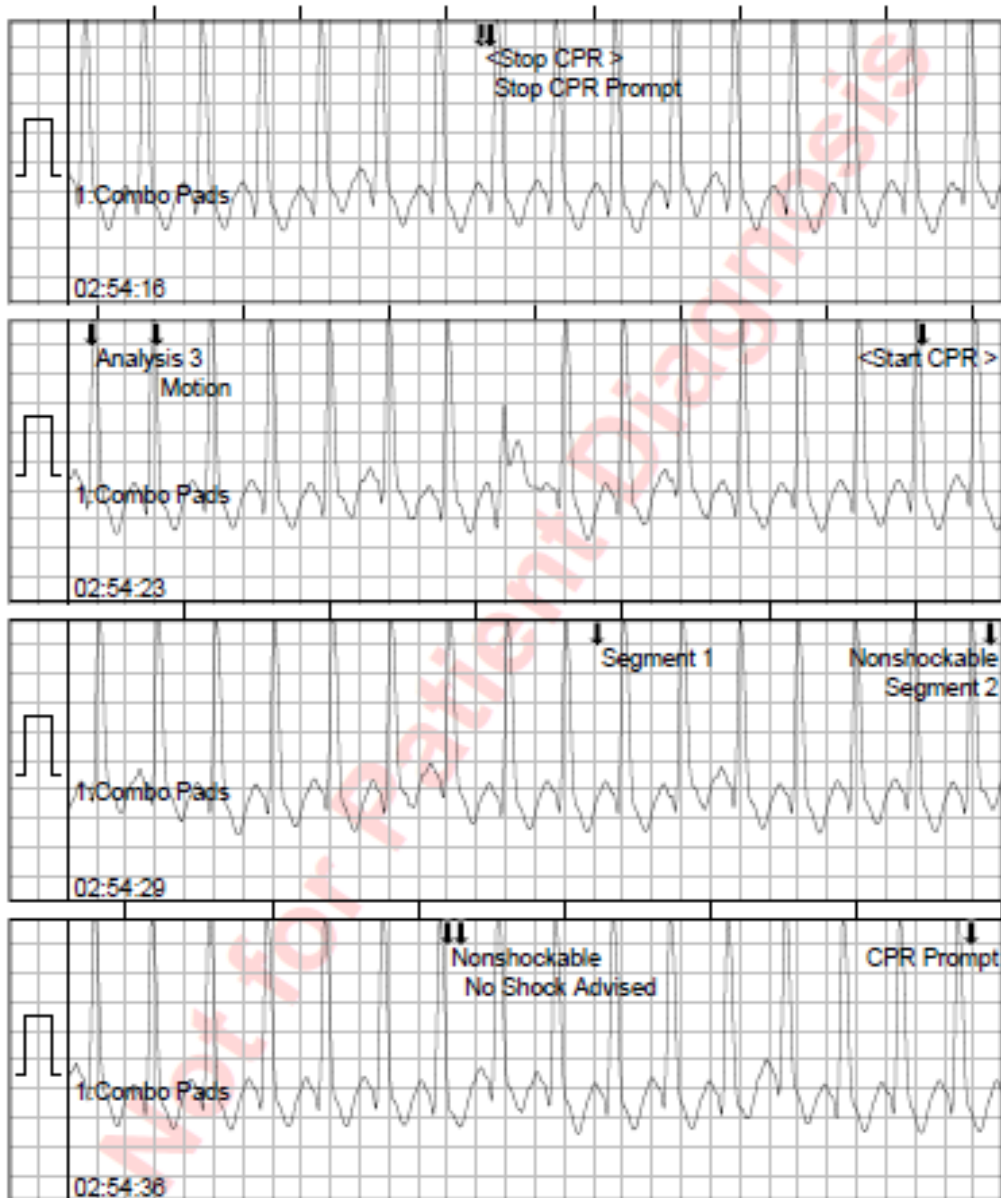

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.



Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.



Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.

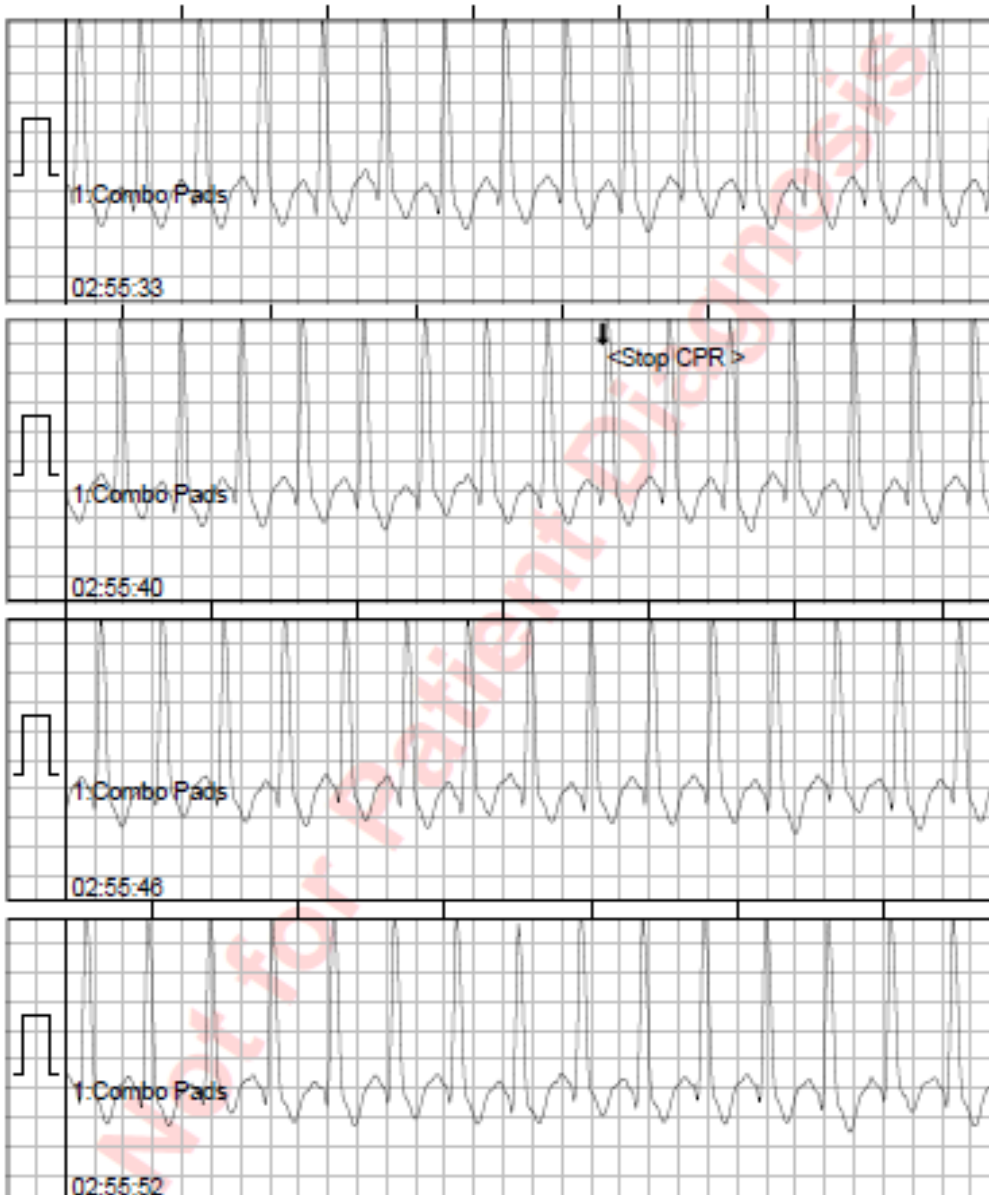

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.



Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

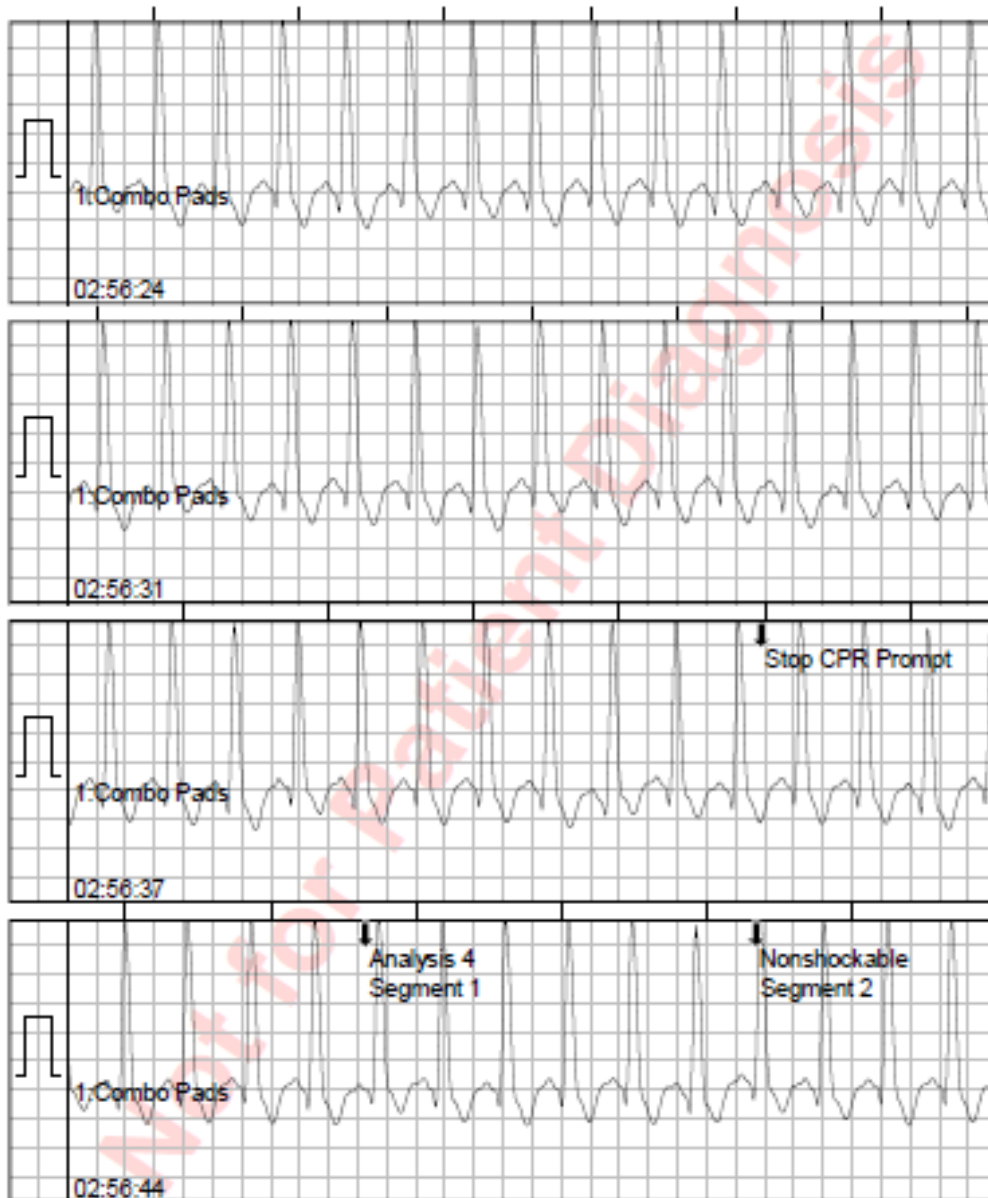

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

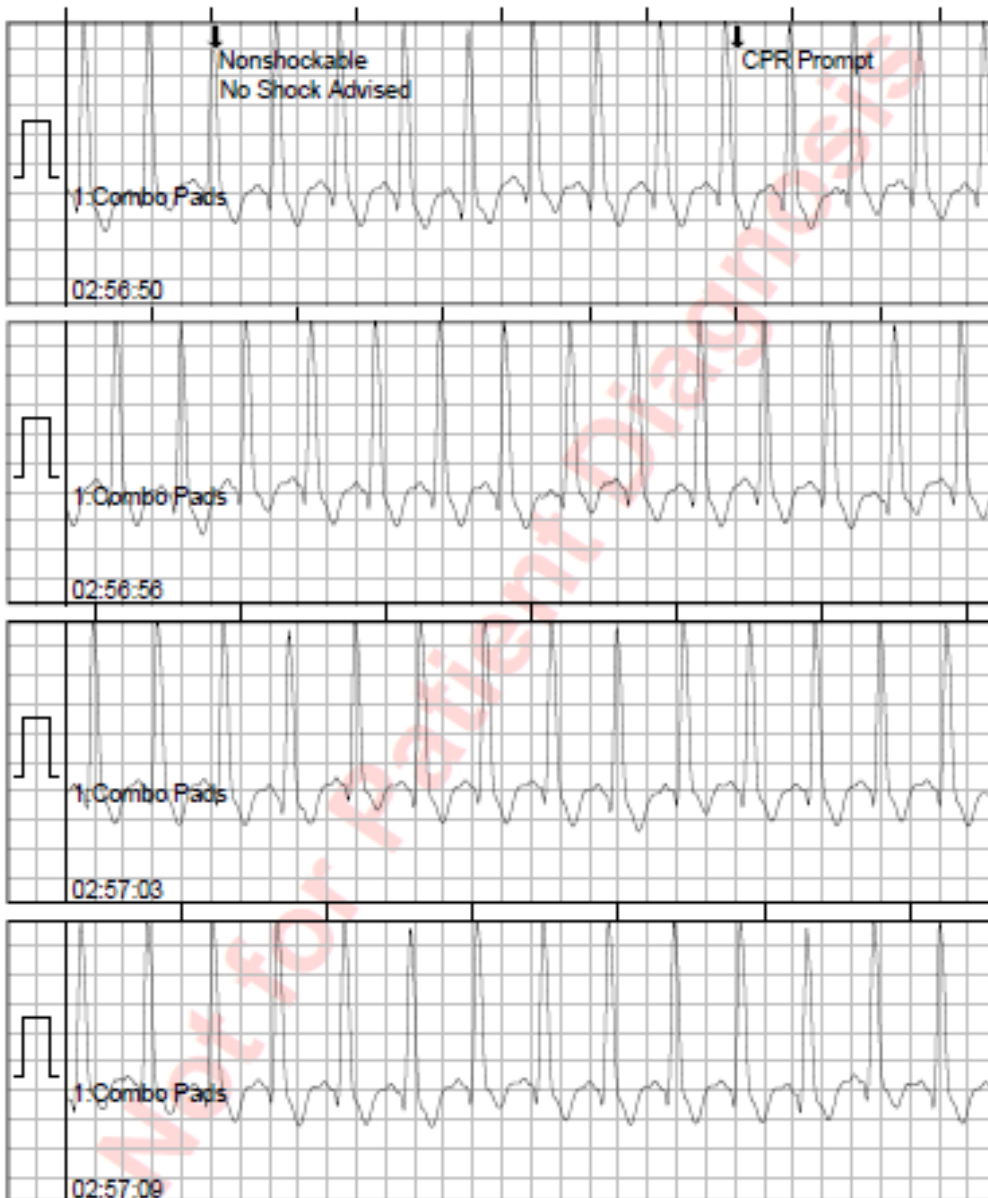

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

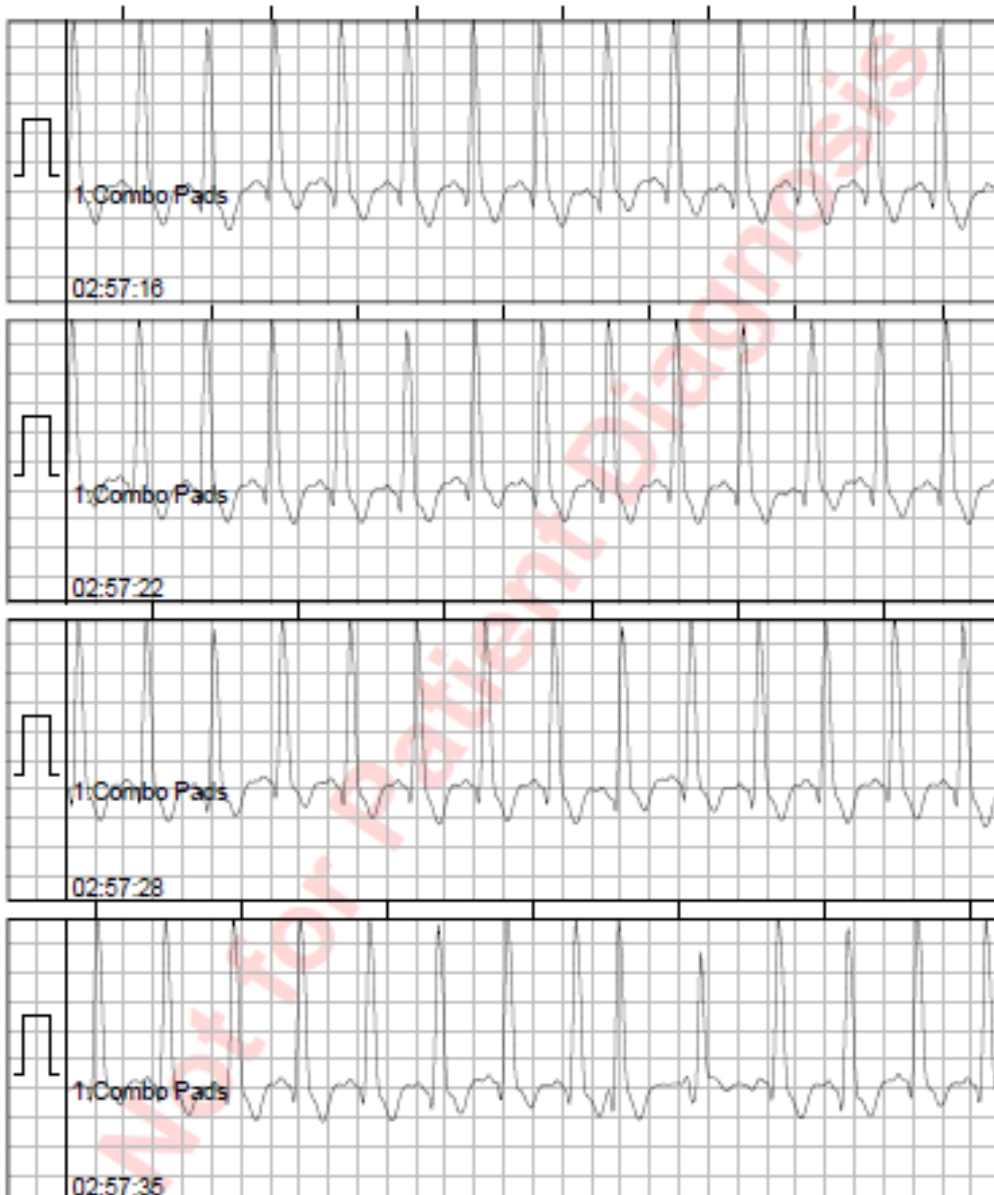

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

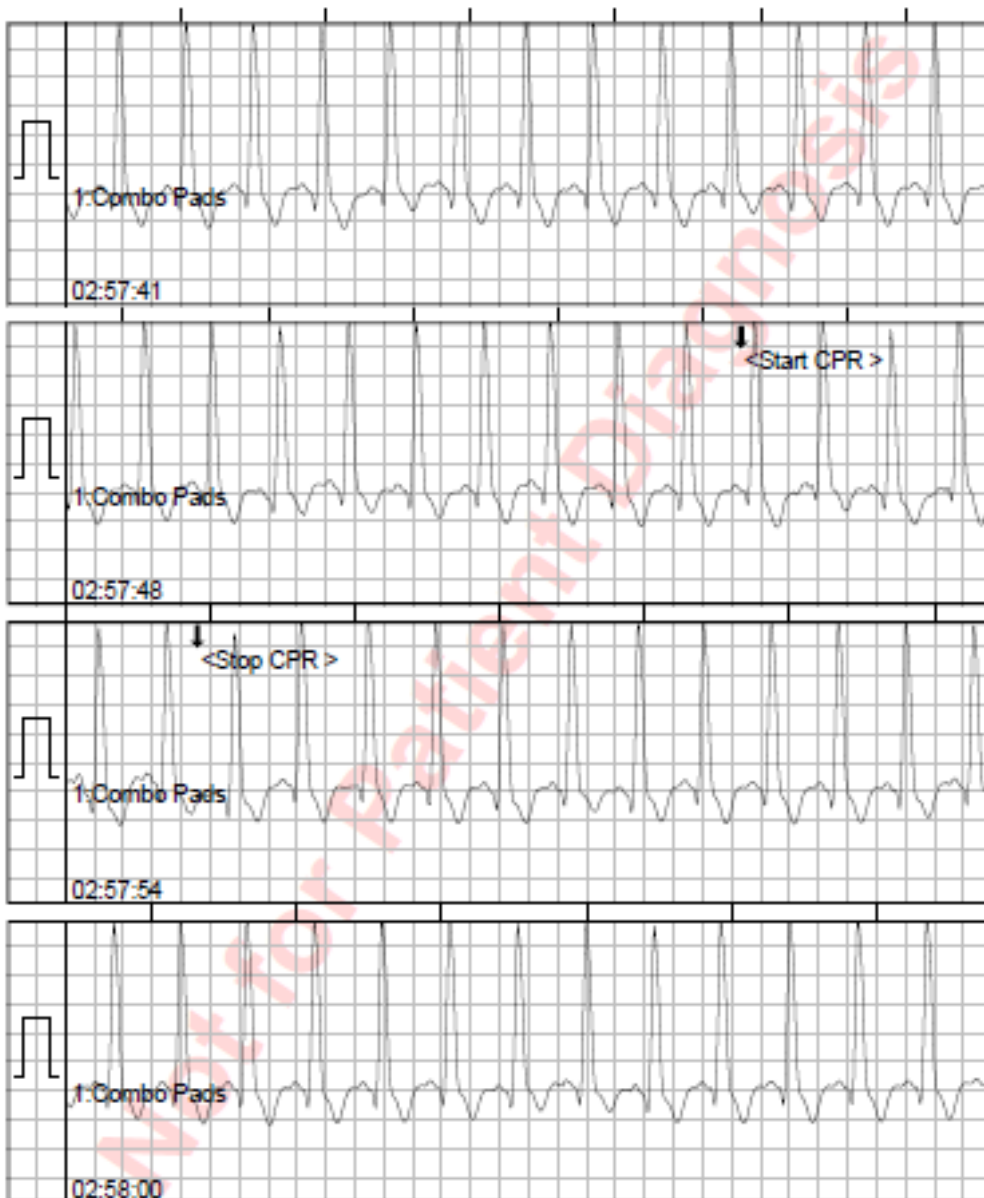

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

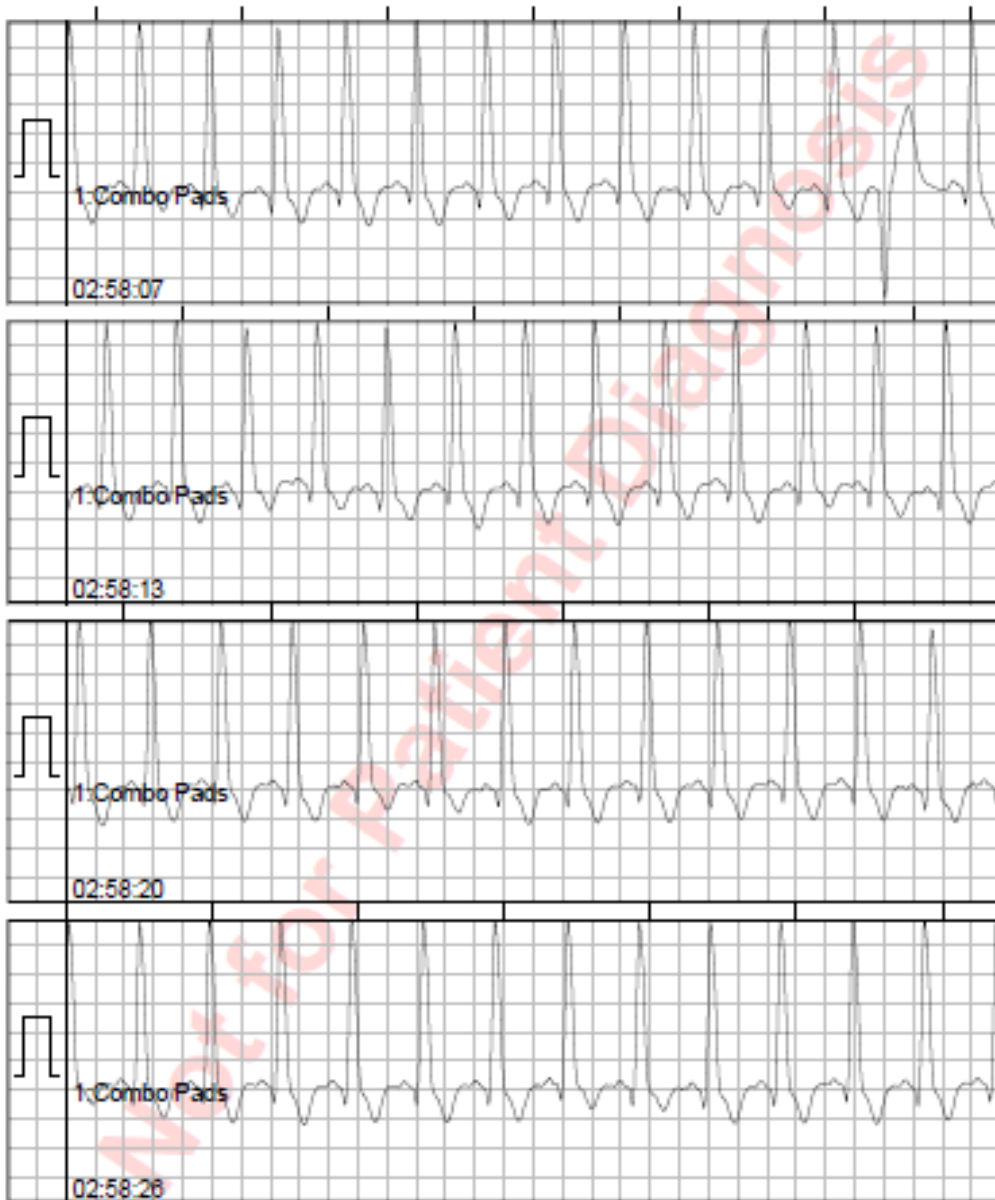

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

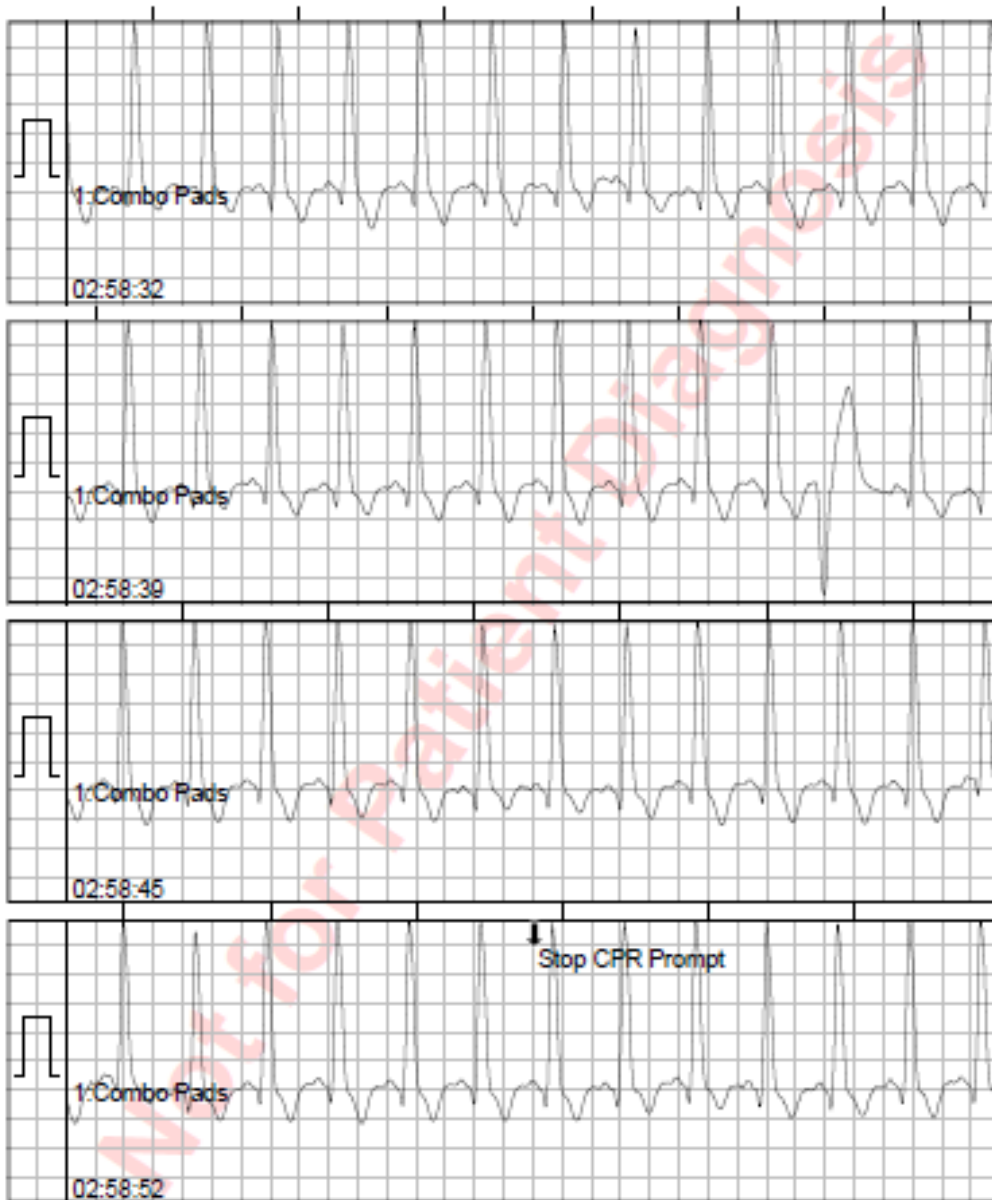

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		


*Times have been adjusted by the system.

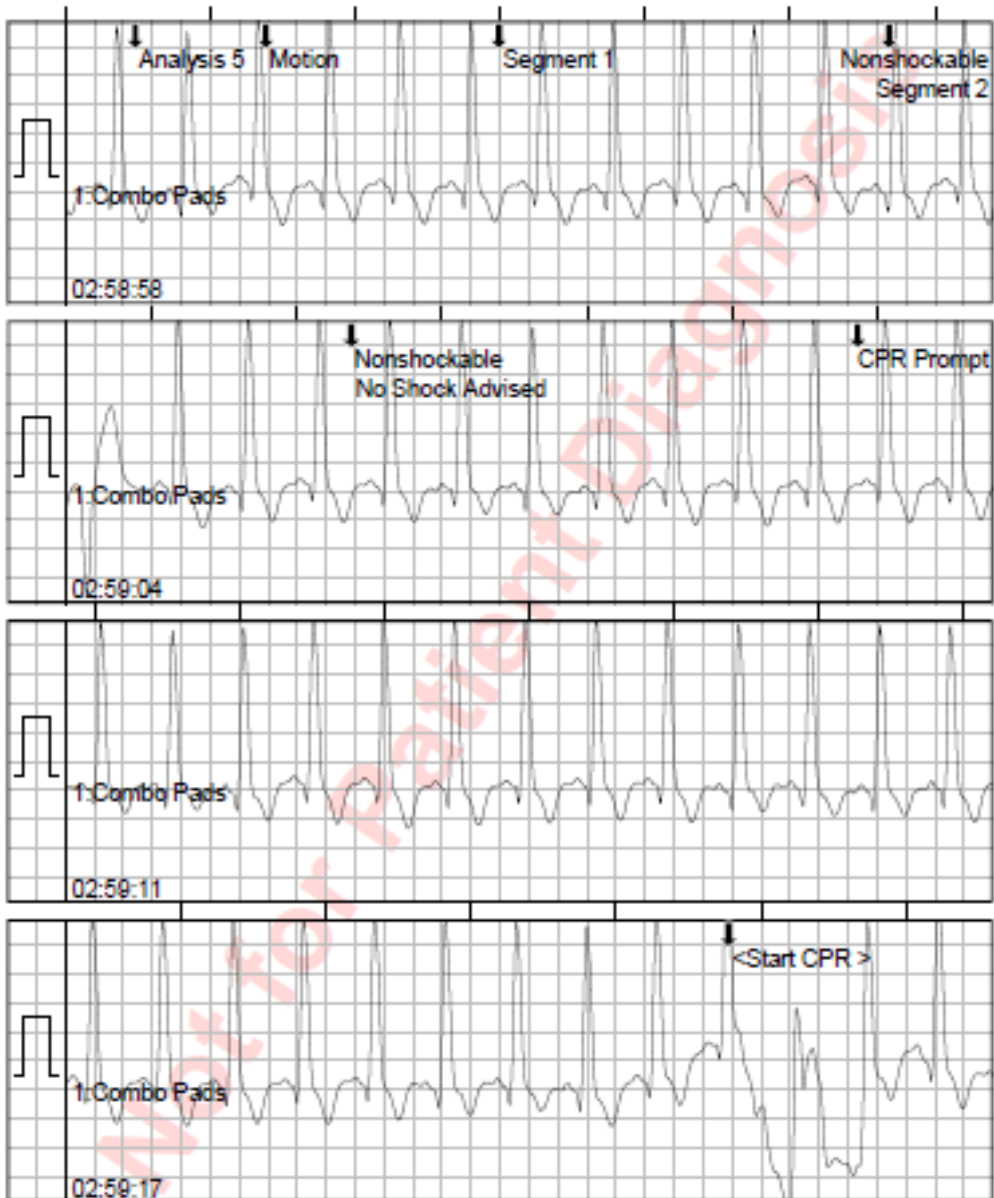

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.

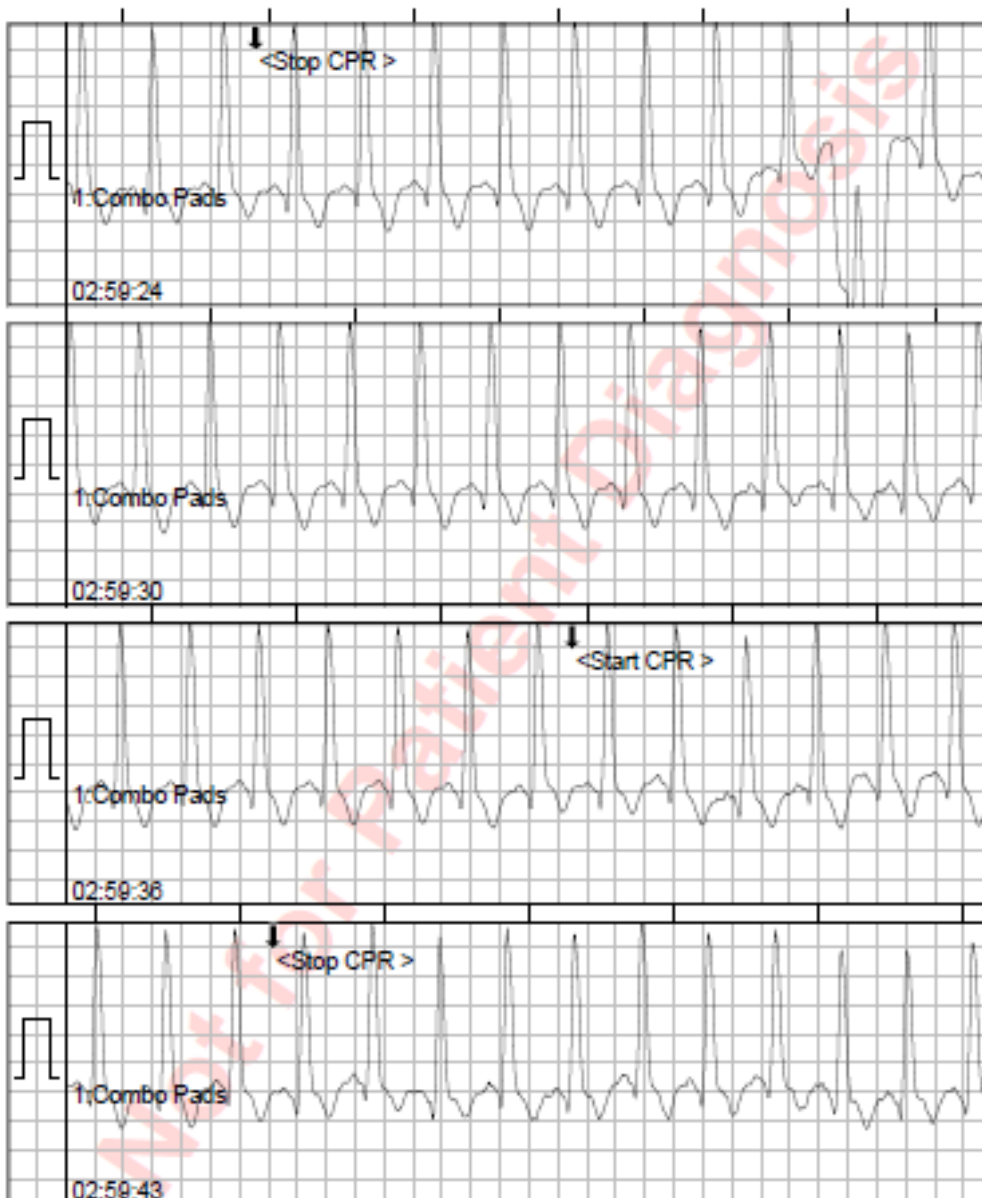

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.



2015-06-03 11:09:34

Your Institution Name

Page of 39

Continuous Complete

Incident ID:	2015053117483000-43365359	Device Type:	LPCRP
Patient ID:	2015053117483000-LPCRP43365359	Device ID:	43365359
Patient Name:		Device Serial Number:	LPCRP43365359
Power On:	2015-06-01 02:48:18	Device Configuration:	00000048A2200000000
Speed/Size:	25mm/sec / x1,0	Software Version:	3202124-035 REV 3.13
Frequency:	Paddles (,5-21Hz)		

*Times have been adjusted by the system.

